INSTRUCTION MANUAL FOR BOILING STERILIZER BS-1836

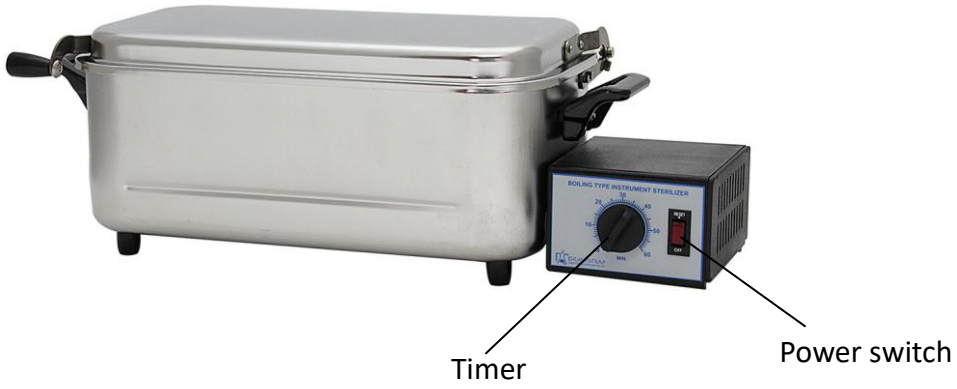

Steps:

1. Fill the sterilizer with 3000 cc (3 liter) water or until it reaches the instrument tray and all sterilizing objects are well immersed.
2. Check the local main voltage which should confirmed with the voltage 220V of the sterilizer before plugging. Turn the 'Power switch' on.
3. Set the 'Timer' to 20 minutes for water to boil and sterilize the instruments.
4. The timer switch will automatically shut –off , when it reaches the time set.
5. After each use, change to fresh clean water. Don't not use impure and dirty water as it will cause trouble with the safety device. Always keep the container clean.
6. Do not wet the electric power parts. Always keep dry.
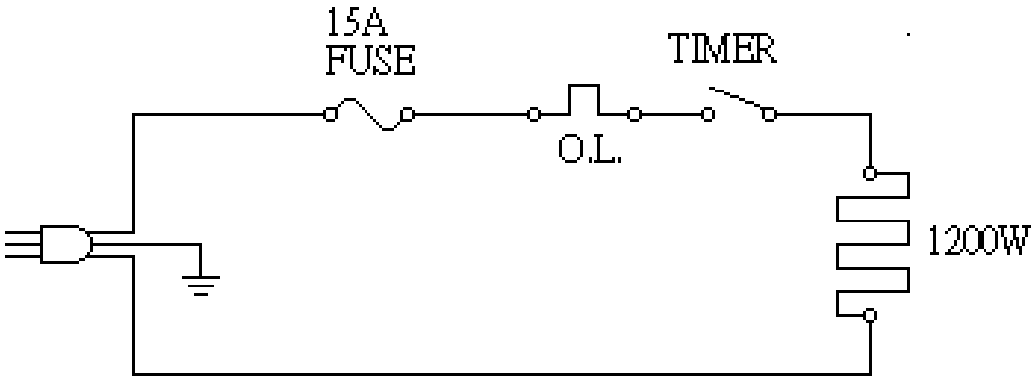
Circuit Diagram: